

# Model LIT MK 720 | with safety equipment for rapid temperature changes


Battery test chambers from BINDER are ideal for aging, performance, and stress testing in quality assurance and battery production. To ensure maximum safety, all the chambers in the LIT MK series are fitted with detection and fire suppression equipment as standard. TÜV SÜD AG has recently confirmed that the LIT MK 240 and LIT MK 720 battery test chambers are suitable for EUCAR LEVEL 6.

## BENEFITS

- Safety thanks to extensive protective measures
- Homogeneous climate conditions thanks to APT.line™ preheating chamber
- Extensive programming and data collection
- Excellent overview of the test object thanks to large heated viewing window



Model 720

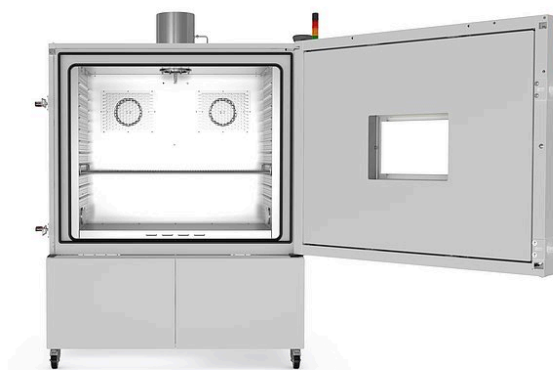

Model 720

## MAIN FEATURES

- Temperature range: -40 °C to +110 °C
- Class 2 independent temperature safety device when temperature is set to +120 °C
- Reversible stainless steel pressure relief flap installed in the middle on top of the unit
- Enhanced door-locking mechanism with reinforced brackets
- Monitoring of CO, H<sub>2</sub>, O<sub>2</sub>, and temperature in testing area atmosphere
- Inertization equipment
- CO<sub>2</sub> fire suppression
- APT.line™ preheating chamber technology
- Programmable condensation protection for samples
- Heated viewing window with LED interior lighting
- BINDER Multi Management Software APT-COM™ basic edition
- Intuitive touchscreen controller with time-segment and real-time programming
- Internal data logger, measured values can be read out in open format via USB
- 2 access ports with silicone plugs, 80 mm, left and right
- Class 2 independent adjustable temperature safety device (DIN 12880) with visual alarm
- Computer interface: Ethernet
- 1 stainless steel rack, can be freely positioned
- CFC-free refrigerant R-452A
- Cooling with compressor cooling unit
- TÜV SÜD confirms that the LIT MK 240 and LIT MK 720 chambers are suitable for EUCAR level 6

## OPTIONAL EQUIPMENT

- Electromechanical door-locking mechanism
- Additional access ports available in various sizes and locations
- Multi Management Software APT-COM for managing, recording, and documenting unit parameters
- Services – wide range of services to ensure that the unit functions correctly

## ORDERING INFORMATION

| Interior volume [L] | Voltage           | Option model                         | Version         | Art.-No.  |
|---------------------|-------------------|--------------------------------------|-----------------|-----------|
| 734                 | 400 V 3~ ph 50 Hz | Standard                             | LITMK720-400V   | 9020-0403 |
|                     | 480 V 3~ ph 60 Hz | with voltage and frequency converter | LITMK720-480V-C | 9020-0405 |

## TECHNICAL DATA


| Description  | LITMK720-400V <sup>1</sup> | LITMK720-480V-C <sup>1</sup> |
|--|----------------------------|------------------------------|
| <b>Article Number</b>  | <b>9020-0403</b>           | <b>9020-0405</b>             |
| <b>Performance Data Temperature</b>                          |                            |                              |
| Temperature range  | -40...110                  | -40...110                    |
| Temperature fluctuation depending on setpoint [± K]          | 0.1...0.5                  | 0.1...0.5                    |
| Average heating-up rate according to IEC 60068-3-5 [K/min]   | 4                          | 4                            |
| Average cooling down time according to IEC 60068-3-5 [K/min] | 3.4                        | 3.4                          |
| Max. heat compensation at 25 °C [W]                          | 3600                       | 3600                         |
| <b>Electrical data</b>                                       |                            |                              |
| Rated Voltage [V]  | 400                        | 480                          |
| Power frequency [Hz]   | 50                         | 60                           |
| Nominal power [kW]   | 8.7                        | 8.7                          |
| Unit fuse [A]  | 16                         | 16                           |
| Phase (Nominal voltage)                                      | 3~                         | 3~                           |

1 All technical data is specified for unloaded units with standard equipment at an ambient temperature of +22 °C ±3 °C and a power supply voltage fluctuation of ±10 %. The temperature data is determined in accordance to BINDER factory standard following DIN 12880, observing the recommended wall clearances of 10 % of the height, width, and depth of the inner chamber. Technical data refers to 100 % fan speed. All indications are average values, typical for units produced in series. We reserve the right to change technical specifications at any time.

| Description  | LITMK720-400V <sup>1</sup> | LITMK720-480V-C <sup>1</sup> |
|--|----------------------------|------------------------------|
| Article Number   | 9020-0403                  | 9020-0405                    |
| <b>Measures</b>  |                            |                              |
| Interior volume [L]  | 734                        | 734                          |
| Net weight of the unit (empty) [kg]                          | 570                        | 522                          |
| Permitted load [kg]  | 160                        | 160                          |
| Load per rack [kg]   | 40                         | 40                           |
| Viewing window width [mm]                                    | 508                        | 508                          |
| Viewing window height [mm]                                   | 300                        | 300                          |
| Wall clearance back [mm]                                     | 300                        | 300                          |
| Wall clearance sidewise [mm]                                 | 200                        | 200                          |
| <b>Internal Dimensions</b>                                   |                            |                              |
| Width [mm]   | 1200                       | 1200                         |
| Height [mm]  | 1020                       | 1020                         |
| Depth [mm]   | 600                        | 600                          |
| <b>Doors</b>   |                            |                              |
| Unit doors   | 1                          | 1                            |
| <b>Housing dimensions not incl. fittings and connections</b> |                            |                              |
| Width net [mm]   | 1794                       | 1794                         |
| Height net [mm]  | 2005                       | 2005                         |
| Depth net [mm]   | 1186                       | 1186                         |
| <b>Environment-specific data</b>                             |                            |                              |
| Sound-pressure level [dB(A)]                                 | 65                         | 67                           |
| <b>Fixtures</b>  |                            |                              |
| Number of shelves (std./max.)                                | 1/11                       | 1/11                         |

<sup>1</sup> All technical data is specified for unloaded units with standard equipment at an ambient temperature of +22 °C ±3 °C and a power supply voltage fluctuation of ±10 %. The temperature data is determined in accordance to BINDER factory standard following DIN 12880, observing the recommended wall clearances of 10 % of the height, width, and depth of the inner chamber. Technical data refers to 100 % fan speed. All indications are average values, typical for units produced in series. We reserve the right to change technical specifications at any time.

### DIMENSIONS incl. fittings and connections [mm]

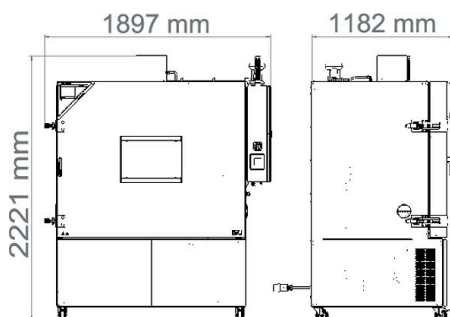

## OPTIONS

| Designation                                     | Description  | *  | Art.-No.  |
|---|--|----|-----------|
| <b>Access port with silicone plug</b>           | left   |    |           |
|   | 30 mm  | 01 | 8012-1322 |
|   | 50 mm  | 01 | 8012-1328 |
|   | 80 mm  | 01 | 8012-1334 |
|   | 100 mm   | 01 | 8012-1542 |
|   | 125 mm   | 01 | 8012-1351 |
|   | top  |    |           |
|   | 80 mm  | 01 | 8012-1536 |
|   | 100 mm   | 01 | 8012-1530 |
|   | 125 mm   | 01 | 8012-1533 |
| <b>Analog output 4-20 mA</b>                    | for temperature values (output not adjustable)   | -  | 8012-1084 |
| <b>Calibration certificate, expanded</b>        | for temperature; for extending the measurement in center of chamber to include another test temperature      | -  | 8012-1124 |
| <b>Calibration certificate, temperature</b>     | for temperature, measurement in center of chamber at specified temperature                                   | -  | 8012-1143 |
|   | temperature measurement incl. certificate and 27 measuring points at specified temperature                   | -  | 8012-1602 |
|   | temperature measurement incl. certificate, 15- 18 measuring points at specified temperature                  | -  | 8012-1581 |
|   | temperature measurement incl. certificate, 9 measuring points at specified temperature                       | -  | 8012-1560 |
| <b>Compressed air connection</b>                | for the connection to an existing pressurized air network  | -  | 8012-1797 |
| <b>Door lock</b>                                | lockable door handle   | -  | 8012-1861 |
| <b>Electromechanical door-locking mechanism</b> | Controlled via control contact in time program or manually   | -  | 8012-2011 |
| <b>Heated access port</b>                       | On left side, including locking latch and silicone plug  |    |           |
|   | 150 mm diameter  | -  | 8012-1999 |
| <b>Locking latch for access port plug</b>       | For securing the silicone plug of an access port   |    |           |
|   | 30 mm diameter   | -  | 8012-2012 |
|   | 50 mm diameter   | -  | 8012-2013 |
|   | 80 mm diameter   | -  | 8012-2014 |
|   | 100 mm diameter  | -  | 8012-2015 |
|   | 125 mm diameter  | -  | 8012-2016 |
| <b>Notch-type access port</b>                   | notch-type access port in door, 100 x 35 mm  | -  | 8012-1851 |
| <b>Pt 100 temperature sensor</b>                | additional flexible Pt 100, interior, for displaying the temperature on the unit display                     | -  | 8012-1093 |
| <b>Reinforced boiler base</b>                   | for increasing the load capacity of the interior base<br>to 300 kg   | -  | 8012-2010 |
| <b>RS 485 interface, 2-wire</b>                 | Additional serial interface can be used parallel to Ethernet, for Multi Management Software APT-COM™         | -  | 8012-1768 |
| <b>Zero voltage relay contacts</b>              | for controlling 3 relay contacts via program regulators, accessible via 6-pin DIN socket (max. 24 V - 2.5 A) | -  | 8012-1095 |

\* Notes › See last page

## ACCESSORIES

| Designation                            | Description   | * | Art.-No.  |
|--|---|---|-----------|
| <b>APT-COM™ 4 GLP-Edition</b>          | for working under GLP-compliant conditions. Measured values are documented in a tamper-proof way in line with the requirements of FDA Regulation 21 CFR 11.<br>version 4, GLP edition | - | 9053-0042 |
| <b>APT-COM™ 4 PROFESSIONAL-Edition</b> | convenient unit and user management built on the BASIC edition. Suitable for networking up to 100 units.<br>version 4, PROFESSIONAL edition   | - | 9053-0040 |
| <b>pH-neutral detergent</b>            | concentrated, for gentle remove of residual contaminants; 1 kg  | - | 1002-0016 |

\* Notes › See last page

| Designation                                | Description  | * | Art.-No.  |
|--|--|---|-----------|
| <b>Qualification documents</b>             | IQ/OQ documents – supporting documents for validation performed by customers, consisting of: IQ/OQ checklists incl. calibration guide and comprehensive unit documentation; parameters: temperature, CO <sub>2</sub> , O <sub>2</sub> , pressure, depending on unit  |   |           |
|  | Digital in PDF format  | – | 7057-0001 |
|  | Hard copy inside folder  | – | 7007-0001 |
|  | IQ/OQ/PQ documents – supporting documents for validation performed by customers, according to customer requirements, PQ section added to qualification folder IQ/OQ; parameters: temperature, CO <sub>2</sub> , O <sub>2</sub> – or pressure, depending on unit  |   |           |
|  | Digital in PDF format  | – | 7057-0005 |
|  | Hard copy inside folder  | – | 7007-0005 |
| <b>Rack</b>                                | stainless steel  | – | 8012-2054 |
| <b>Rack accessories</b>                    | fasteners (1 set of 4) for additional security of racks  | – | 8012-0620 |
| <b>Rack, reinforced</b>                    | stainless steel, with fasteners (1 set of 4)   | – | 8012-0684 |
| <b>RS 485 / RS 422 interface converter</b> | RS 422 cable set and RS 485 / RS 422 interface converter for connection to 10-way plug distributor   |   |           |
|  | 115 V option model   | – | 8012-0599 |
|  | 230 V option model   | – | 8012-0589 |
| <b>Shelf, perforated</b>                   | Stainless steel  | – | 8009-0511 |
| <b>WLAN kit</b>                            | The kit contains a client bridge that establishes a wireless connection between BINDER units and APT-COM4, LIMS, or customer-specific software via an Ethernet interface. It provides an alternative solution in situations where units need to be positioned in locations without an on-site Ethernet connection. In secured networks, installation and configuration must be performed by the customer's IT service. | – | 8500-0164 |

\* Notes › See last page

## SERVICES

| Designation   | Description  | *          | Art.-No.  |
|---|--|------------|-----------|
| <b>Installation services</b>                                      |  |            |           |
| Unit commissioning  | Connect the unit to the customer-side connections (electricity, water, wastewater, gas), basic functions check, brief operating instructions. (excl.: unpacking, setup, controller instructions, programming, installation work)   | 05         | DL10-0310 |
| Unit instructions   | Instruction regarding operating principle and basic functions of the unit, operation of the control electronics including programming  | 05         | DL10-0710 |
| <b>Maintenance contracts</b>                                      |  |            |           |
| <b>Maintenance services</b>                                       |  |            |           |
| GOLD 3-year maintenance contract                                  | Maintenance service as contractually agreed, visual inspection of mechanical and electrical components, check of control response, 20% discount on spare parts, testing of all key functions, replacement of wear parts, calibration of one temperature/humidity value, including certificate                  | 05         | DL20-0950 |
| Leakage test  | Testing and logging of the leak-tightness of systems containing hydrofluorocarbons in accordance with Regulation EC842/2006, incl. test book   | 05         | DL00-0034 |
| Maintenance   | One-off maintenance service in accordance with maintenance schedule. Visual inspection of mechanical and electrical components, testing of all key functions. Calibration of a test temperature specified by the user in center of usable space without certificate  | 05         | DL20-0510 |
| SILVER 3-year maintenance contract                                | Maintenance service as contractually agreed, visual inspection of mechanical and electrical components, check of control response, 20% discount on spare parts, testing of all key functions, calibration of one test temperature specified by the user in the center of the usable space, without certificate | 05         | DL20-0840 |
| <b>Calibration services</b>                                       |  |            |           |
| Calibration certificate, temperature                              | Calibration of one (1) test temperature specified by the user in center of chamber, including certificate  | 03, 04, 05 | DL30-0101 |
|   | Extension of calibration of one (1) additional test temperature specified by the user in the center of the usable space, including certificate   | 03, 04, 05 | DL30-0102 |
| O <sub>2</sub> , CO <sub>2</sub> , and H <sub>2</sub> calibration | O <sub>2</sub> , CO <sub>2</sub> , and H <sub>2</sub> calibration at specified values, measurements are taken with analyzed test gas, including certificate  | 03, 04, 05 | DL30-0403 |
| Temperature measurement, 18 measuring points                      | Temperature measurement with 18 measuring points with a set value specified by the user, including certificate   | 03, 04, 05 | DL30-0118 |
| Temperature measurement, 27 measuring points                      | Temperature measurement with 27 measuring points with a set value specified by the user, including certificate   | 03, 04, 05 | DL30-0127 |

\* Notes › See last page

| Designation                                 | Description   | *          | Art.-No.  |
|---|---|------------|-----------|
| Temperature measurement, 9 measuring points | Temperature measurement with 9 measuring points with a set value specified by the user, including certificate | 03, 04, 05 | DL30-0109 |
| <b>Validation services</b>                  |   |            |           |
| Execution of IQ/OQ                          | Execution of IQ/OQ in accordance with qualification folder  | 05         | DL41-0200 |
| Execution of IQ/OQ/PQ                       | Execution of IQ/OQ/PQ in accordance with qualification folder   | 05         | DL44-0500 |

\* Notes › See last page

## NOTES

- 01 Condensation may occur in the area around the access port. Access ports may be placed in custom locations for an additional charge.
- 02 UL mark is not granted when this option is used.
- 03 Sensor calibration is performed in an accredited calibration laboratory.
- 04 Calibration is performed according to the BINDER factory standard.
- 05 Quoted prices do not include travel costs. Please refer to the chapter on BINDER Service for travel costs for your region. Quoted prices for services performed in Switzerland do not include a country-specific added fee (available on request).

### **BINDER GmbH**

Tuttlingen, Germany  
TEL +49 7462 2005 0  
FAX +49 7462 2005 100  
info@binder-world.com  
www.binder-world.com

### **BINDER Asia Pacific (Hong Kong) Ltd.**

Kowloon, Hong Kong, P.R. China  
TEL +852 39070500  
FAX +852 39070507  
asia@binder-world.com  
www.binder-world.com

### **Representative Office for CIS**

Moscow, Russia  
TEL +7 495 988 15 16  
FAX +7 495 988 15 17  
russia@binder-world.com  
www.binder-world.com

### **BINDER Environmental Testing Equipment (Shanghai) Co., Ltd.**

Shanghai, P.R. China  
TEL +86 21 685 808 25  
FAX +86 21 685 808 29  
china@binder-world.com  
www.binder-world.com

### **BINDER Inc.**

Bohemia, NY, USA  
TEL +1 631 224 4340  
FAX +1 631 224 4354  
usa@binder-world.com  
www.binder-world.us